

epServices
for premium performance



Pipette Service Done Right

Eppendorf Pipette Calibration

»Are Your Results Reliable?«

Global quality standards assured with premium services by the experts

Your pipettes are high precision instruments, and require regular maintenance and checks to stay in peak performance. Especially the precision and accuracy of your pipettes are important to ensure the quality of your downstream results. When your pipettes are not working in peak condition, your experimental results can come into question.

Therefore, regular maintenance, calibration, and adjustment services by Eppendorf will help identify potential issues, and assure your pipettes and dispensers continue to generate reproducible results. Our new, globally available pipette service portfolio always follows the latest and strict international quality standards for calibration. Various calibration options include a thorough check of the pipette internally and externally, ensuring that wearable parts like O-rings are replaced in a timely manner.




Calibration Drift Due to Wear and Tear

Month to month over a yearlong testing period, the new pipette in standard lab use is calibrating within the error limits as shown in the graph. However, wear and tear is causing this pipette's calibration to continuously just trend


towards the upper limit. Without any maintenance, calibration or adjustment measures, this pipette will eventually fall out of calibration, potentially causing questionable and unreliable results.

Example pipette calibration over time

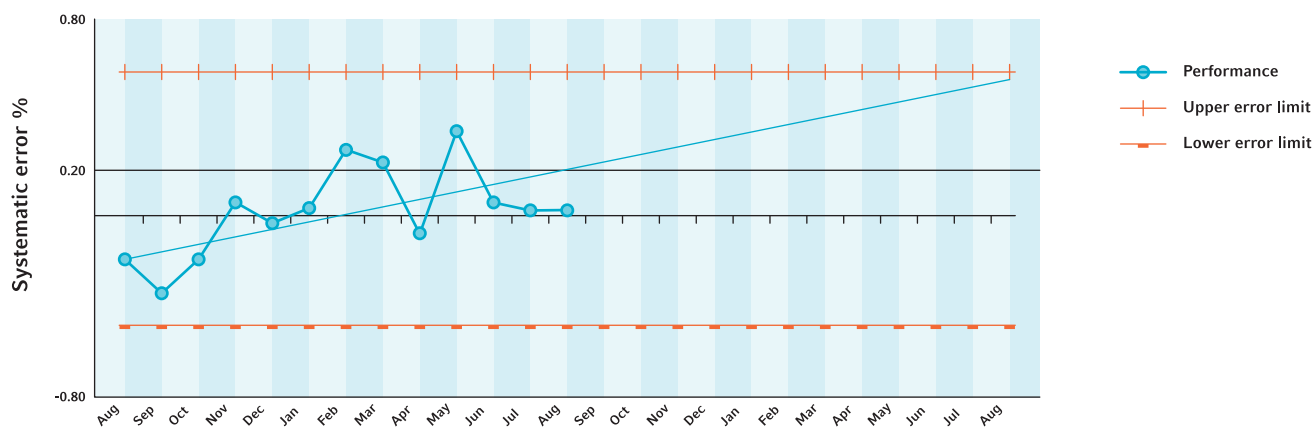

What Else is Important?


Calibrating with 3 volumes to compensate for the non-linear correlation of error and volume

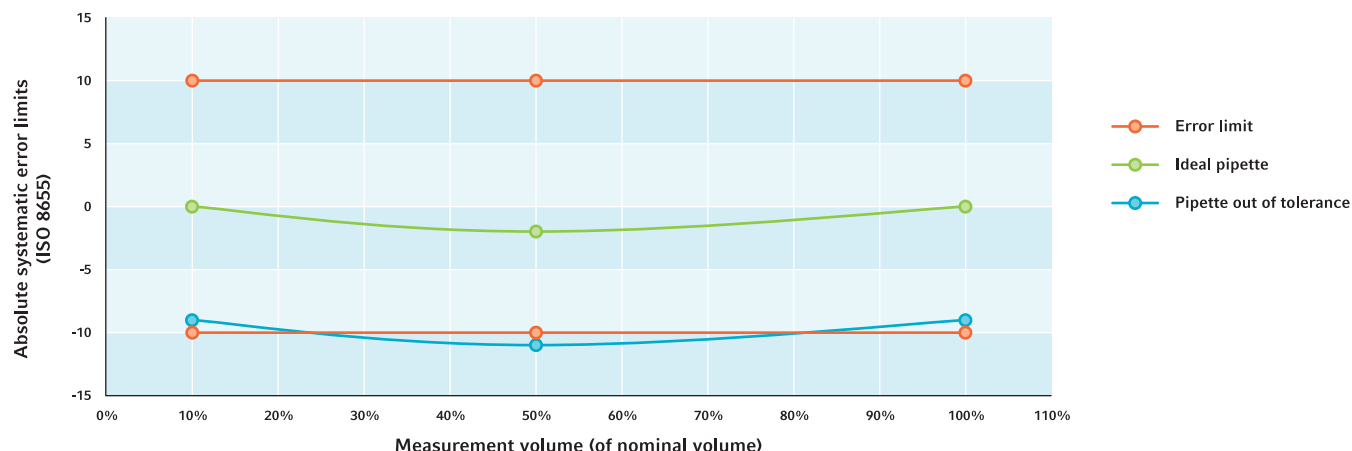

ISO 8655 requires 3 volumes to be tested during calibration: Nominal volume, 50% of nominal volume, and lower limit of useful volume or 10% of nominal volume (whichever is the greater). Since the error limits of a pipette are not linear from minimum to maximum volume, it is possible to have the 10% and 100% volumes perform within the systematic error limits while the 50% volume does not.

The graph above demonstrates this phenomenon with the blue line representing a pipette that is out of tolerance. The user would not know that this pipette isn't functioning properly without testing all 3 volumes.

Calibrating with 10 measurements versus 4 measurements to compensate for deviations

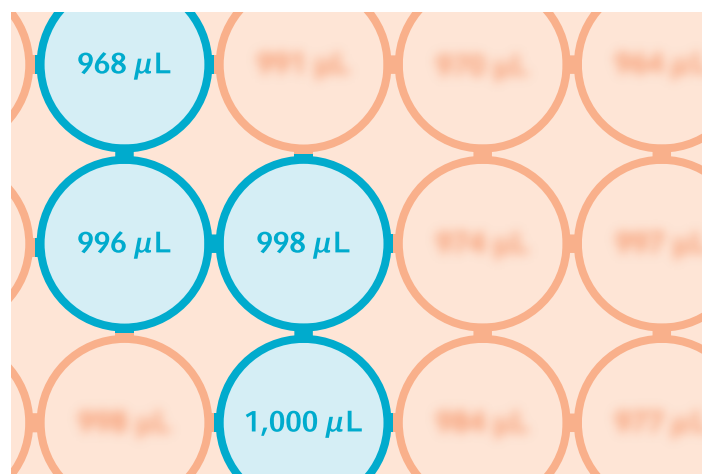

The boxes above represent a set of calibration measurements from a 1.000 μL pipette. On the left, taking only 4 measurements produces an error of 0.3%, well within the pipette's 0.6% error limit. On the right, taking all 10 measurements



produces an error of 1.6%, considerably outside the pipette's 0.6% limits. More confidence in the calibration is produced and the results become statistically more accurate when using 10 measurements as recommended by ISO 8655.

Why Eppendorf Pipette Service?




Beyond ISO Conformity

We maintain over 5000 pipette manufacturer specifications and conform to the manufacturer standard when their specifications are tighter than ISO 8655 standards, if requested by customer.



Highly Trained Service Technicians

Our highly-qualified technicians go through 200 hours of training and must pass rigorous exams to become certified before servicing pipettes.

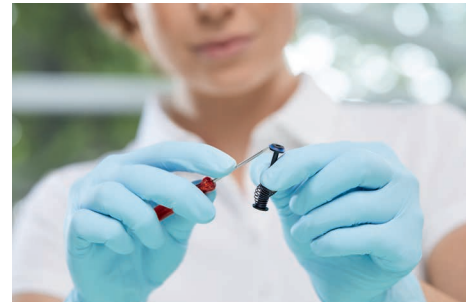

Thorough Maintenance

Our calibration services include a thorough check of the pipette internally and externally, ensuring that wearable parts like O-rings are replaced in a timely manner.

eppendorf

Kalibrierschein / Calibration Certificate
 erstellt durch die Kalibrierlaboratorien der
 Eppendorf Vertrieb Deutschland GmbH

Standorte:
 Bornholmerweg 1 Im Thal 4 Marzthamer Straße 1 Magnusstraße 11 Peter-Herlein-Straße 2
 22339 Hamburg 82377 Penzberg 69115 Heidelberg 12489 Berlin 50389 Wesseling-Berzdorf

akkreditiert nach DIN EN ISO/IEC 17025:2018
 accredited according DIN EN ISO/IEC 17025:2018




Mitglied im / Member of
 Deutschen Kalibrierdienst **DKD**

Kalibrierzeichen
 Calibration mark

2183902-00
 D-K
 15057-61-00
 2020-10



Seite 2 von 2 Seiten zum Kalibrierschein

2183902-00
D-K
15057-61-00
2020-10

Location of calibration:
 Eppendorf Vertrieb Deutschland GmbH, Hamburg

Calibration subject:
 Calibration certificate No. 2183902-00
 Calibration name: Eppendorf
 Volume range: 0.10 - 2.00 µl
 Serial No.:
 Test Lab:

Type of pipette: Automatic
 Division ID No.:
 Used by: Eppendorf AG, P.O. Box

Calibration procedure: Test according to DIN EN ISO 8655 - DKD-R 8-1

Measurement results		Test volume		Test volume		Test volume		Test volume	
0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl	0.25 µl
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.251	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.251	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.251	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250
0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250	0.250

Caption: 1. Labeled Volume

Fully Accredited Service Centers

In our major markets, ISO 17025 accredited calibration processes are available in the field or at the service center. As a liquid handling expert partner, we can help you meet any regulatory need.

Over 60 Years of Experience

Since we released the first piston stroke pipette in 1961, we continue to manufacture and service pipettes with a passion for improving user results.

Audit-proof Documentation

Our calibration documentation will give you peace of mind due to reduced workload for your qualification and regulatory audit process. Most of our calibration facilities worldwide use our CFR21 part 11 compliant software.

Eppendorf Calibration Process

Decontamination

After verifying the customer's declaration of decontamination, all pipettes go through an additional Eppendorf decontamination process before they are forwarded to our calibration facilities.



Preventive Maintenance and Repair

- > As found examination and calibration if requested
- > Cleaning of external and inner parts and maintenance (lubricating, exchange of wear and tear parts if necessary) of the devices
- > Leak testing
- > Performing necessary repairs



Calibration and Adjustment

- > Usage of high-precision single- and multi-channel balances fulfilling ISO 8655 requirements
- > Usage of original manufacturer pipette tips
- > Measurement according to ISO 8655
- > Evaluation according to manufacturer specifications (if requested to ISO 8655 or customer SOP error limits)
- > Adjustment, if device is outside of the error limits
- > ISO 17025 calibration certificate on request.



Labeling and Packaging

- > Device is packed with calibration certificate and service report ready for shipment
- > Each device is labeled with a calibration service sticker with the calibration date
- > Shipping in secure packaging with our certified shipping partners assures the pipette arrives in peak condition.



Frequently Asked Questions

How often should you calibrate a pipette?

> You decide within the scope of your quality standards on the calibration frequency. The frequency of calibration may vary depending on the number of users, the frequency of use of the pipettes, as well as the type of dispensed liquids and the accepted tolerances. A renewal of the conformity by ISO 8655 is recommended at least once per year.

What is a renewal of a conformity?

> The calibration/renewal of conformity consists of a pipette maintenance and an As-Left calibration. These strictly adhere to ISO 8655 criteria, ensuring that the pipette meets conformity to ISO 8655 requirements or even tighter specifications like manufacturer specifications.

What happens, if my instrument cannot be repaired?

> We will inform you and offer you an attractive trade-in offer.
> On request we will dispose your old instrument or send it back to you.

What is an ISO 17025 calibration certificate?

> An ISO 17025 calibration certificate not only contains the data from the calibration protocol, but also contains the measurement uncertainty, and the accreditation confirmation of the lab. The ISO 17025 calibration certificate with the included raw data information ensures the traceability chain for the calibration.

Why do I need a calibration without preventive maintenance in addition?

> The As-Is protocol is performed before the As-Left calibration or renewal of conformity including maintenance. This protocol shows the calibration status of the pipette as received from the user, and is indicative of the pipette's performance prior to the renewal of conformity.



> Watch video:
www.eppendorf.com/pipette-video

Service Center, On-Site Service or On-Site Pick Up!



Treat your pipettes well with premium services from the expert!

Precision and accuracy of your pipettes are important to ensure the quality of your results. Regular maintenance, calibration, and adjustment services by Eppendorf assure your pipettes and dispensers continue to deliver reproducible results.

Our new and clearly designed calibration services thoroughly check your pipettes inside and out to ensure wearable parts like O-rings are replaced in a timely manner. We offer a range of service options from an economic calibration to a certified calibration service in our ISO 17025 accredited laboratory located in Sydney.

Need your pipettes calibrated? Get excited...

With a wide range of options available, on-site service options, on-site pick up options and fast return times, contact your local Eppendorf Service Center for more information.

Get what you want - Know what you get! Contact: service@eppeppendorf.com.au

Why choose us?

- > Highly qualified and experienced technical staff
- > Backed by 60 years of liquid handling experience
- > Accredited to local and international standards
- > Superior customer service and support
- > Unmatched in-house turnaround time
- > Range of calibration options where pipette performance can be evaluated according to Manufacturer specifications, ISO 8655 or customised specifications



Qualification and
Certification

ISO 8655

ISO 8655 defines the standard criteria by which a pipette should be calibrated and which maximum permissible error limits should be used at each volume. ISO 8655 criteria includes measurements at 3 volumes, 10 measurements at each volume, and controls for room environment.

ISO 17025

The ISO 17025 accreditation certifies the high level of competence and compliance with strict quality rules. ISO 17025 criteria include a traceability chain for measurement equipment, measurement uncertainty values, and approved quality standards.

Pipette Calibration Service

Calibration Services – Ordering information

Service	Calibration measurements	Calibration measurements	Decontamination from outside ²	Checking, cleaning, lubricating ³ before calibration	Single channel pipette/dispenser	4-channel pipette	6-channel pipette	8-channel pipette	12-channel pipette	16-channel pipette	24-channel pipette
ISO 8655 including PM ⁵ (Standard)		10 per test volume ¹	included	included	0082000142	0082000342	0082000343	0082000165	0082000166	0082000185	0082000186
3x4 without PM ⁵ (As found)	4 per test volume ¹		included		0082000139	0082000336	0082000337	0082000159	0082000160	0082000179	0082000180
3x4 including PM ⁵ (Basic)		4 per test volume ¹	included	included	0082000141	0082000340	0082000341	0082000163	0082000164	0082000183	0082000184

Calibration Service Packages – Ordering information

Service	Calibration measurements	Calibration measurements	Outside decontamination ² ; checking, cleaning, lubrication ⁴	ISO 17025 Accreditation calibration certificate	Single channel pipette/dispenser	4-channel pipette	6-channel pipette	8-channel pipette	12-channel pipette	16-channel pipette	24-channel pipette
ISO 8655 Verified (As found/Standard)	4 per test volume ¹	10 per test volume ¹	included		0082000234	0082000324	0082000325	0082000235	0082000236	0082000237	0082000238
ISO 17025 including PM ⁵ (As found/Standard)		10 per test volume ¹	included	included	0082000143	0082000326	0082000327	0082000167	0082000168	0082000187	0082000188
ISO 17025 Advanced (As found/Standard/NATA)	4 per test volume ¹	10 per test volume ¹	included	included ³	0082000227	0082000322	0082000323	0082000228	0082000229	0082000230	0082000231

Additional Services – Ordering information

ISO 17025 Calibration Certificate	0082000211
Advanced Documentation, Excel file for calibration information on all pipettes/dispensers per order	0082000212

¹ 10%, 50% and 100% of nominal volumes for variable volume instruments. ² Pipettes and dispensers and package equipment need to be decontaminated before sending in. ³ ISO 17025 accreditation calibration certificate is included in the second calibration after the maintenance. ⁴ Internal parts. ⁵ Preventative Maintenance.

Additional Services Charges

On-site calibration services in your own laboratory	Inquire
Labor Charge, 15 min. of repair services, time unit of one technician	0082000210

Download a decontamination form at www.eppendorf.com/epServices.

Your local distributor: www.eppendorf.com/contact

Eppendorf South Pacific Pty. Ltd. · Level 1, 97 Waterloo Road · Macquarie Park, NSW 2113 · Australia
info@eppendorf.com.au · www.eppendorf.com

www.eppendorf.com/epservices