


# Optimal Organisation for Your Biosafety Cabinet



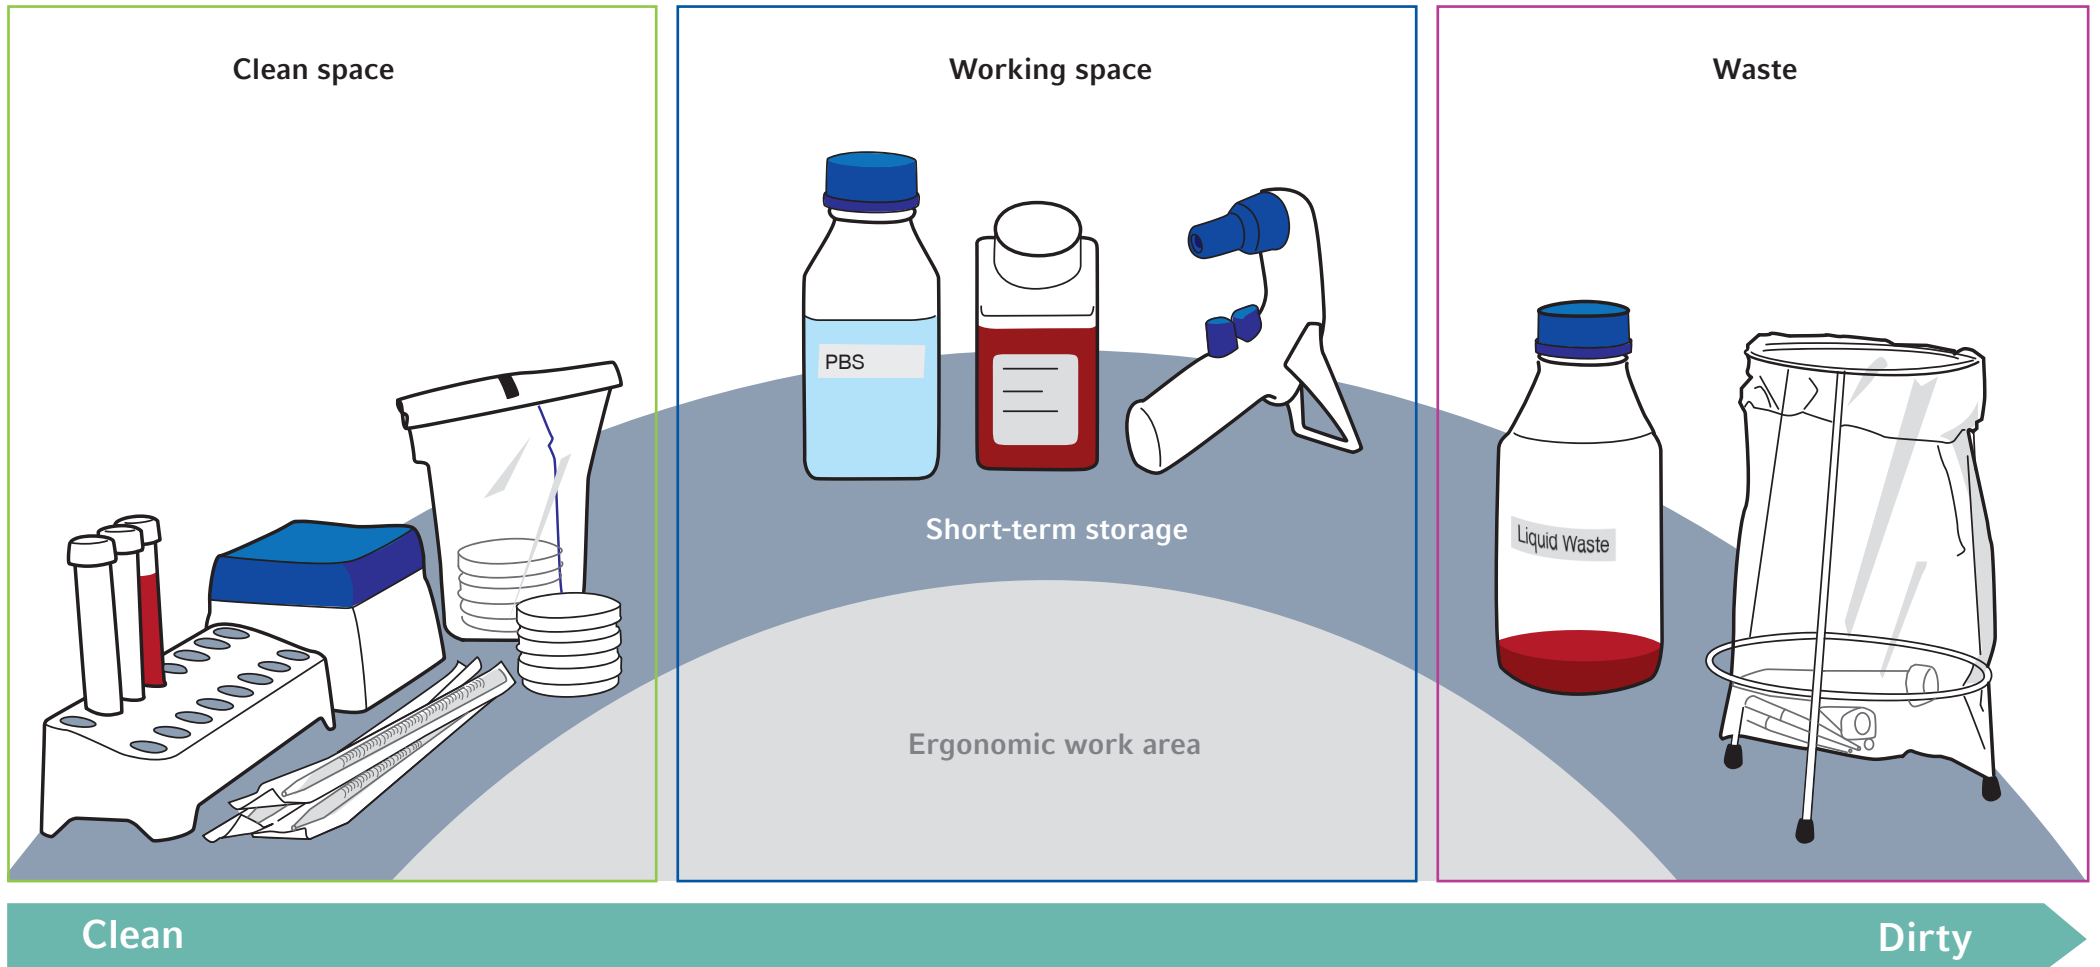

# Cleaning Schedule Biosafety Cabinets

Laminate for reuse

When?	What?	Disinfection reagent*	How?*	Check UV lamp	Who?	Comments
Date	Device (e.g. left hood)	What was used for disinfection?	Cleaning/disinfection of exterior, interior, and removable parts		Name	Special occurrences, observations, incidents etc. (e.g. UV lamp replaced)

Maintenance Interval: \_\_\_\_\_

Room: \_\_\_\_\_

\* According to manufacturer’s instructions