



New Brunswick™ Excella® E-10 Open Air Shaker

Operating manual

Copyright © 2014 Eppendorf AG, Germany. No part of this publication may be reproduced without the prior permission of the copyright owner.

The company reserves the right to change information in this document without notice. Updates to information in this document reflect our commitment to continuing product development and improvement.

Eppendorf® and the Eppendorf logo are registered trademarks of Eppendorf AG, Germany.

New Brunswick™ and the New Brunswick™ logo are trademarks of Eppendorf AG, Germany.

Excella® is a registered trademark of Eppendorf, Inc., USA.

Trademarks are not marked in all cases with ™ or ® in this manual.

Table of contents

1	Operating instructions	5
1.1	Using this manual	5
1.2	Danger symbols and danger levels	5
1.2.1	Hazard icons	5
1.2.2	Degrees of danger	5
1.3	Symbols used	5
2	Safety	7
2.1	User profile	7
3	Product description	9
3.1	Main illustration	9
3.2	Overview	9
4	Installation	11
4.1	Inspection and unpacking	11
4.2	Selecting the location	11
4.3	Electrical requirements	12
4.4	Installing a platform	12
4.5	Install flask clamp	13
4.6	Electrical connections	15
5	Operating controls and function	17
5.1	Control panel	17
5.1.1	Status indicators	17
5.1.2	LED display	18
5.1.3	Function indicators	18
5.1.4	User interface keys	19
6	Operation	21
6.1	Start/Stop	21
6.2	Continuous (untimed) run	21
6.3	Check setpoint	21
6.4	Timed functions	21
6.5	Alarm Functions	22
6.6	Power Failure	22
6.7	Speed Calibration	23
7	Troubleshooting	25
7.1	Troubleshooting guide	25
8	Maintenance	27
8.1	Cleaning external surfaces	27
9	Technical data	29
9.1	Specifications	29

Table of contents

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

10	Ordering information	31
10.1	Parts and accessories	31
10.1.1	Belt replacement parts	31
10.1.2	Dedicated platforms	31
10.1.3	Universal platform flask capacity	31
10.1.4	Racks and trays	32
11	Transport, storage and disposal	33
11.1	Disposal	33
12	Declaration of conformity	35
	Index	37






1 Operating instructions

1.1 Using this manual

- ▶ Carefully read this operating manual before using the device for the first time.
- ▶ Also observe the operating manual enclosed with the accessories.
- ▶ The operating manual should be considered as part of the product and stored in a location that is easily accessible.
- ▶ When passing the device on to third parties, be sure to include this operating manual.
- ▶ If this manual is lost, please request another one. The latest version can be found on our website www.eppendorf.com (international) or www.eppendorfn.com (North America).

1.2 Danger symbols and danger levels

1.2.1 Hazard icons

	Electric shock		Crushing
	Material damage		Hazard point
	Heavy loads		

1.2.2 Degrees of danger

The following danger levels are used in safety messages throughout this manual.


DANGER	<i>Will</i> lead to severe injuries or death.
WARNING	<i>May</i> lead to severe injuries or death.
CAUTION	May lead to light to moderate injuries.
NOTICE	May lead to material damage.

1.3 Symbols used

Example	Meaning
▶	You are requested to perform an action.
1. 2.	Perform these actions in the sequence described.
•	List.

Operating instructions

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Example	Meaning
	References useful information.

2 Safety

2.1 User profile



CAUTION!

- ▶ This equipment must be operated as described in this manual. If operational guidelines are not followed, equipment damage and personal injury can occur. Please read the entire Operating Manual before attempting to use this unit.
 - ▶ Do not use this equipment in a hazardous atmosphere or with hazardous materials for which the equipment was not designed.
 - ▶ Eppendorf is not responsible for any damage to this equipment that may result from the use of an accessory not manufactured by Eppendorf.
-

Safety

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

3 Product description

3.1 Main illustration

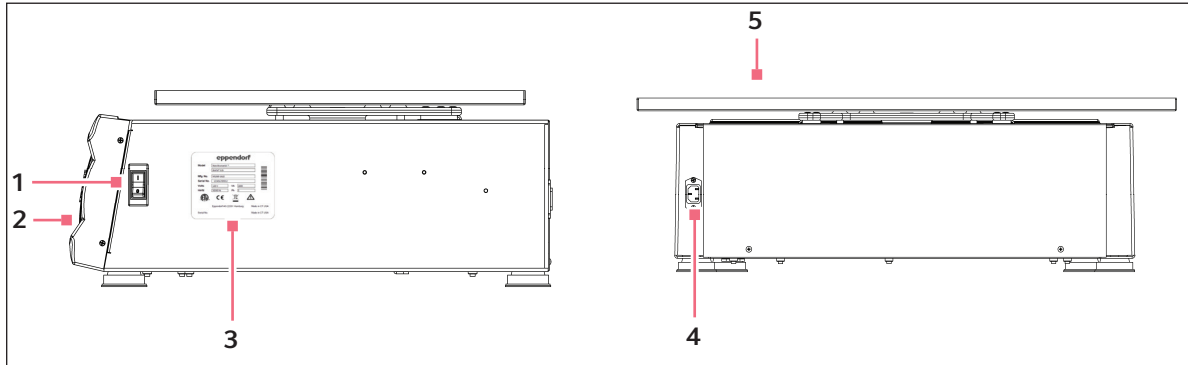


Fig. 3-1: Excella E-10 side and rear view

1 ON/OFF switch

2 Control panel

3 Electrical specification plate

4 Power receptacle

5 Platform

3.2 Overview

The Excella E-10 is a portable benchtop shaker utilizing a UniCentric™ single eccentric counterbalanced drive to provide horizontal plane rotary motion in a 2.54 cm (1 in) circular orbit. A Proportional/Integral (PI) Microprocessor controller with instantaneous digital feedback controls the speed over a range of 50 rpm – 400 rpm .

The shaker may be operated either continuously or in a timed mode via a programmable timer for shaking periods of 0.1 – 99.9 h.

The E-10 is equipped with visual and audible alarms which are activated when an alarm condition exists, as follows:

- The end of a timed run
- Deviations of shaking speed
- Power failure

A wide variety of platforms can be used with the E-10. Dedicated platforms are available for a variety of flask sizes. Universal platforms, and test tube racks are also available.

Product description

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

4 Installation

4.1 Inspection and unpacking

Inspection of Boxes

After you receive your order from Eppendorf, inspect the boxes carefully for any damage that may have occurred during shipping. Report any damage immediately to the carrier and to your local Eppendorf Sales Order Department.

Packing List Verification

Verify against your packing list that you have received the correct materials.

Unpacking of Equipment



WARNING!

- ▶ The E-10 is heavy. Two or more people are required to lift the shaker.



CAUTION!

- ▶ There are two small plastic straps that held the bearing housing in place during shipping. Once the shaker is unpacked and inspected, remove the straps from the bearing housing.
-

4.2 Selecting the location



WARNING!

- ▶ Do not position the equipment so that it is difficult to unplug from the mains/power.
-

Physical Location

It is essential that the instrument be situated in a area where there is sufficient space for the shaker and platform to clear walls and obstructions during operation.

The surface on which the E-10 is placed must be smooth, level, and able to support the shaker under full load operating conditions.

Installation

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Operating Environment

The shaker is designed to operate optimally in the following ambient conditions:

- 5 – 45 °C
- 20 – 80 % Relative Humidity non-condensing
- Up to 2000 m

4.3 Electrical requirements

The Excella E-10 can be equipped to run on:

- 100/120 volts, 50/60 Hz, 1500 VA maximum
- 230 volts, 50/60 Hz, 1500 VA maximum

In all cases, voltage variations must not exceed ± 10 %.

4.4 Installing a platform

A platform must be installed on the shaker prior to use.

The shaker is shipped with the four Allen (hexagonal, countersunk) head platform screws installed in the upper bearing housing. These screws must be removed before installing a platform. The Allen key is provided.

**WARNING!**

- ▶ Unplug the shaker before installing the platform.
-

1. Using the 7/32 inch hex wrench provided, remove the four Allen head platform screws from the upper bearing housing.

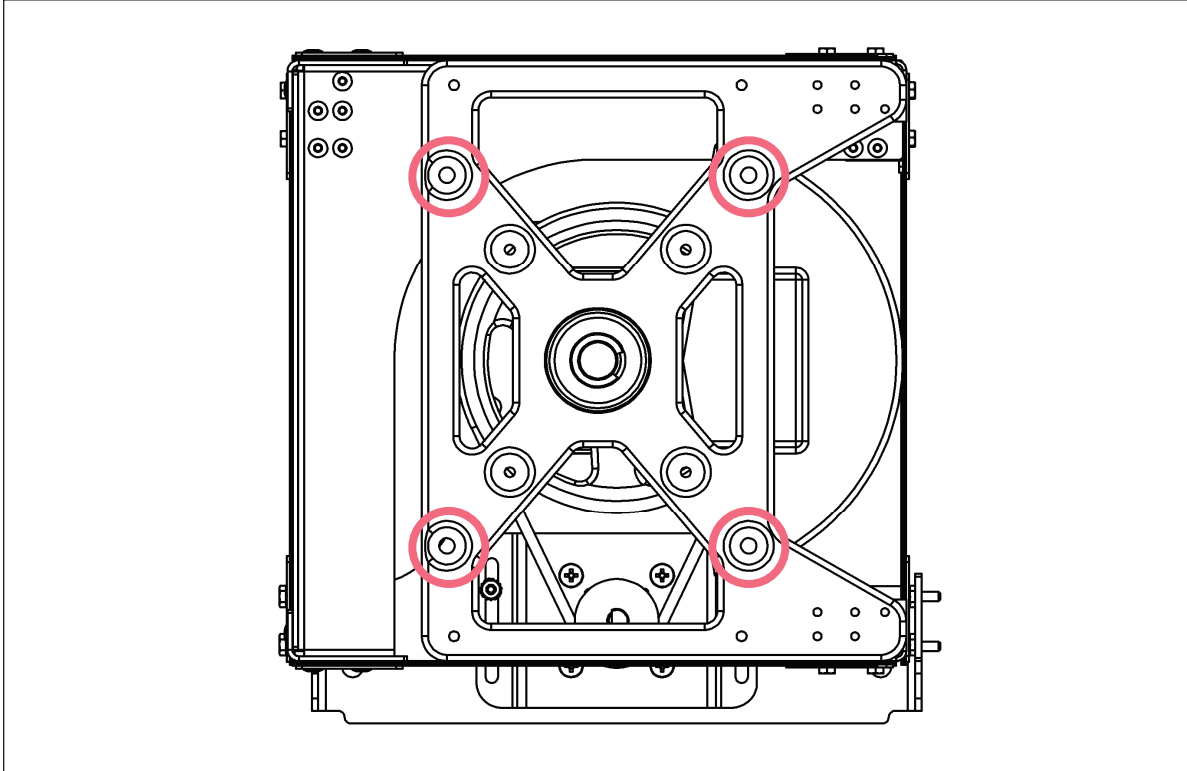


Fig. 4-1: Upper bearing housing with platform screw locations (top view)

2. Place the platform on the UPPER BEARING HOUSING. Align the mounting holes of the platform with the platform screw locations in the upper bearing housing.
3. Insert the four Allen head platform screws previously removed, and tighten them with the 7/32 inch hex wrench provided to secure the platform.

4.5 Install flask clamp

Flask clamps purchased for use with universal platforms require installation (see *Universal platform flask capacity on p. 31*). Clamps are installed by securing the base of the clamp to the platform with the correct type and number of screws. All clamps are shipped complete with hardware.

Clamps for 2 L, 2.8 L and 4 L flasks are shipped with an additional girdle to keep the flasks in place. The girdle is an assembly of springs and sections of rubber tubing. One girdle is already in place on the clamp, the other is packed separately.

Installation

New Brunswick Excella® E-10 Open Air Shaker
English (EN)



NOTICE! Damage to shaker

- ▶ Do not over fill flasks.

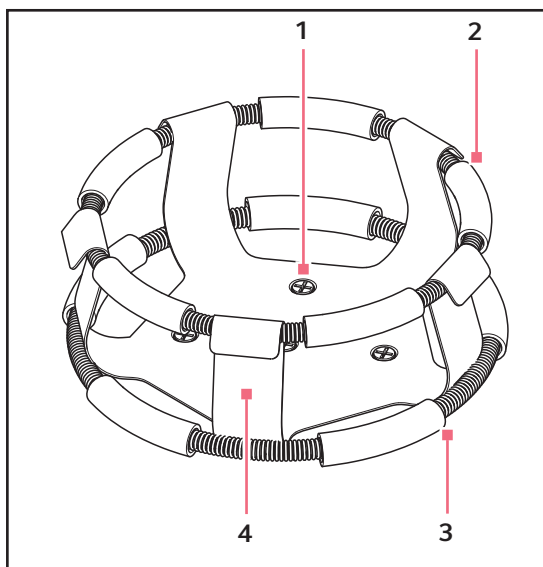


Fig. 4-2: Double girdle clamp

- | | |
|---|--|
| <p>1 Clamp mounting holes (with screws)</p> <p>2 Upper girdle with girdle tubes
Secures the flask within the clamp.</p> | <p>3 Lower girdle with girdle tubes
Prevents the flask from spinning</p> <p>4 Clamp body (legs and base)</p> |
|---|--|


To install these double girdle clamps:

1. Place clamp on platform, aligning its mounting holes with the holes on the platform.
2. Secure the clamp in place using the flat Phillips head screws provided (#S2116-3051, 10-24 × 5/16 in).
3. With the first girdle in place, as delivered, on the upper part of the clamp body, insert an empty flask into the clamp.
4. After making sure the sections of tubing are located between the clamp legs, roll the first girdle down the legs of the clamp as far as it can go.
The tubing sections will rest against the platform, and the springs will be under the clamp base.
5. Place the second girdle around the upper portion of clamp body (just as the first girdle was initially).
6. Make sure that its spring sections rest against the clamp legs, while its rubber tubing sections sit against the flask, in between the clamp legs.



The upper girdle secures the flask within the clamp, and the bottom girdle keeps the flask from spinning.

Eppendorf flask clamps are used on a variety of shaker platforms. Flat head screws of different lengths and thread pitch are used to secure the clamp. To identify the proper screw for your shaker application by reference to the head style, consult the following table, find the proper screws, and set the others aside.

Description	Part No.	Quantity	Application
 10 – 24 × 5/16 in (7.9 mm) flat Phillips head screw	S2116-3051	1	5/16 in (7.9 mm) thick aluminum, phenolic and stainless steel platforms.



The previous table also applies to 2800 ml Fernbach Flask Clamps.

4.6 Electrical connections



CAUTION!

- ▶ A detachable main power cord has been provided with your unit. Only use the cord provided and do not replace cord with an inadequately rated cord.

Before making electrical connections, verify that the power source voltage matches the voltage on the **ELECTRICAL SPECIFICATION PLATE** and that the **ON/OFF SWITCH** is on the **OFF** position. The **ELECTRICAL SPECIFICATION PLATE** and the **ON/OFF SWITCH** are located on the side panel .

Connect the **MAINS/POWER CORD** to the **MAINS/POWER CONNECTOR** on the rear panel and the other end to a suitable, grounded receptacle.

Installation

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

5 Operating controls and function

5.1 Control panel

The control panel consists of the status indicators, LED display, function indicators, and the user interface keys.

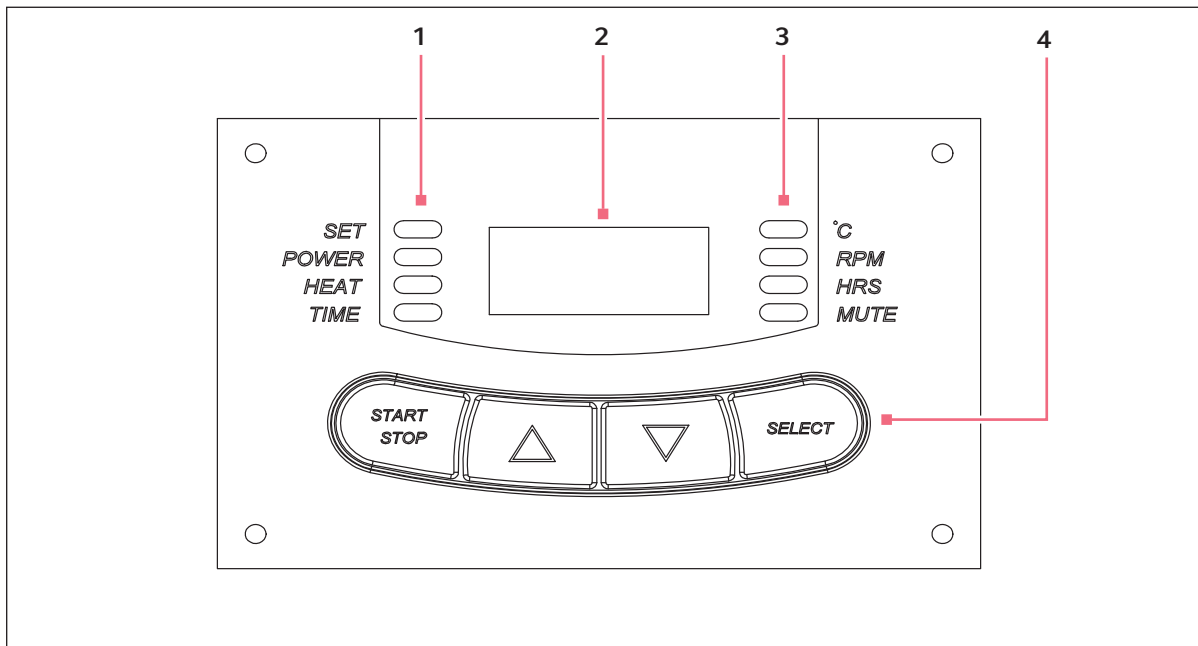


Fig. 5-1: Control panel

1 Status indicators

2 LED display

3 Function indicators

4 User interface keys

5.1.1 Status indicators

4 status indicator lights are located to the left of the LED DISPLAY. They are:

SET	Indicates that the shaker is in the SET MODE, when setpoints are being displayed and can be altered. This is activated by the SELECT key or by pressing the ▲(UP) or ▼(DOWN) KEY.
POWER	Illuminates and blinks during power up or if power is interrupted during a run. Press the SELECT key and change to another function to turn off this indicator.
HEAT*	Illuminates to indicate that the heater is on.
TIME	Indicates that the timer is in operation. The shaker can be programmed to run for a preset time from 0.1 to 99.9 hours. The timer can be disengaged without stopping an ongoing run.

*Not applicable for the E-2, E-5, and E-10

Operating controls and function

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

5.1.2 LED display

The digital display on the control panel is a three-digit LED DISPLAY. During normal operation, the display will indicate:

- Shaker status (On/Off)
- Shaking speed
- Chamber temperature*
- Setpoints
- Hours remaining (in a timed run)
- Lid open ("LID")*

*Not applicable for the E-2, E-5, and E-10

5.1.3 Function indicators

4 function indicator lights are located to the right of the LED DISPLAY. They indicate the current parameter(s) being displayed:

°C*	Interior chamber temperature. Can be set from 4 °C to 60 °C, when in SET MODE, using the ▲(UP) or ▼(DOWN) KEY. It indexes at 0.1 °C increments unless the key is pressed for 4 seconds, after which it indexes more rapidly.
RPM	Revolutions per minute. When in SET MODE, use the ▲(UP) or ▼(DOWN) KEY to change the speed. It indexes at 1 RPM increments unless the key is pressed for 4 seconds, after which it indexes more rapidly.
HRS	Time remaining in a timed run. Can be set from 0.1 to 99.9 hours, in 0.1 increments or, if the ▲(UP) or ▼(DOWN) KEY is pressed for 4 seconds, the time indexes more rapidly. The countdown begins when the START/STOP key is pressed. If the START/STOP key is pressed, the shaking stops (but temperature is maintained) and the timer pauses until the START/STOP key is pressed again. When a timed run ends, the HRS indicator will blink. Press the SELECT key and change to another function to turn off this indicator.
MUTE	This feature is controlled by the SELECT key. When activated, the audible alarm is muted, and remains so until is is reactivated. If MUTE is activated when the shaker is turned off using the ON/OFF switch, it will remain engaged when the machine is powered up again. To activate (or deactivate) the MUTE function, press the SELECT key until the MUTE indicator illuminates; press the ▲(UP) or ▼(DOWN) KEY to display ON or OFF, as desired; then press SELECT.

*Not applicable for the E-2, E-5, and E-10

5.1.4 User interface keys

START/STOP	Start or stop the shaker. It will also activate or stop the timer when a timed run is desired.
SELECT	Used to change the displayed parameter.
▲(UP) or ▼(DOWN)	Used to adjust the setpoint of a displayed parameter up or down. They also allow the user to enter the SET MODE for setpoint changes.

Operating controls and function

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

6 Operation

6.1 Start/Stop

To initially start the shaker:

1. Turn the **ON/OFF SWITCH** to the **ON** position.
During start-up, the **LED DISPLAY** will indicate the model of your shaker.
2. Press the **START/STOP KEY** on the **KEYPAD** to start or stop operation of the platform.
When the shaker begins to operate, the **LED DISPLAY** will track the speed as it accelerates to the last setpoint entered.

6.2 Continuous (untimed) run

1. Press **SELECT** until the RPM INDICATOR is illuminated.
2. If the display indicates that the shaker is OFF, press the **START/STOP KEY**.
3. Press either the **▲(UP)** or **▼(DOWN) KEY** to enter SET MODE.
The SET INDICATOR will illuminate.
4. Set the speed by using the **▲(UP)** or **▼(DOWN) KEY** until the desired setpoint is displayed. Continued pressure the **▲(UP)** or **▼(DOWN) KEY** will cause the setting to change more rapidly.



The setpoint may be changed during a run without stopping the shaker by following Steps 2 – 4 above. During speed changes, a visual alarm (flashing RPM INDICATOR) will flash and an audible alarm will sound until the speed returns to within 5 rpm of the setpoint.

6.3 Check setpoint

1. Press **SELECT** until the desired indicator is illuminated.
2. Briefly press either the **▲(UP)** or **▼(DOWN) KEY** to enter the SET MODE and display the current setpoint.



Holding the **▲(UP)** or **▼(DOWN) KEY** for more than 0.5 seconds causes the speed setpoint to change. Should this occur, resetting will be necessary.

6.4 Timed functions

The shaker may be programmed to automatically stop after a preset time period of 0.1 to 99.9 hours. There must be power to the shaker in order to set the timer, although a timed run can be initiated while the shaker is either stopped or operating.

To set the timer:

1. Press the **SELECT KEY** until the HRS INDICATOR is illuminated.
2. Press either the **▲(UP)** or **▼(DOWN) KEY** to enter the SET MODE and set the desired run time, between 0.1 and 99.9 hours.

Operation

New Brunswick Excella® E-10 Open Air Shaker
English (EN)



If the shaker is stopped, skip to Step 5. If the shaker is already running continue to Step 3.

3. Press the **START/STOP KEY**. The shaker will stop and the display will read OFF.
4. Press the **START/STOP KEY** again; the TIME INDICATOR will light and the shaker will start the timed run.

If the shaker is stopped:

5. Press the **START/STOP KEY**. The shaker will start in untimed mode.
6. Press the **START/STOP KEY** again. The shaker will stop and the display will read OFF.
7. Press the **START/STOP KEY** a third time; the TIME INDICATOR will light and the shaker will start the timed run.

To disable the visual alarm (flashing TIME INDICATOR), press the **SELECT KEY** and change to any other function.

To cancel the timer without stopping the shaker:

Repeat Steps 1 and 2, then immediately press the **START/STOP KEY**. The TIME INDICATOR will cease to flash and the display will read OFF.

6.5 Alarm Functions

In addition to visual alarm, the Excella E-10 has an audible alarm that is activated at predetermined times. It can be deactivated by using the **MUTE** function:

1. Press the **SELECT** key until the MUTE indicator illuminates.
2. Press the **▲(UP) or ▼(DOWN) KEY** to display ON, then press the **SELECT KEY**.

To reactivate the audible alarm:

1. Press the **SELECT** key until the MUTE indicator illuminates.
2. Press the **▲(UP) or ▼(DOWN) KEY** to display OFF, then press the **SELECT KEY**.

6.6 Power Failure

In the event of a power failure, the Excella E-10 is equipped with an automatic restart function.

If the shaker was in operation prior to the power interruption, when power is restored the shaker will begin to operate at its last entered setpoint. The LED DISPLAY will flash and the audible alarm will sound, indicating that a power failure has occurred. Press any key to stop the flashing in the display and the audible alarm.

6.7 Speed Calibration

If speed calibration is needed, contact your local Eppendorf service department.

Calibration mode is entered when pressing and holding the SELECT KEY until the RPM indicator light illuminates. To exit, turn the shaker OFF using the mains/power switch, then turn it back on.

Operation

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

7 Troubleshooting

7.1 Troubleshooting guide

If any problems occur with your shaker, do not attempt to perform any service on the shaker other than specified in this manual. Unauthorized servicing may void the warranty. Please contact your local Eppendorf Service Department.

In any correspondence with Eppendorf, please refer to the Model Number and Serial Number of your shaker. This information is on the **ELECTRICAL SPECIFICATION PLATE**.

There are some problems that you can investigate and correct yourself. Refer to the following Troubleshooting Guide:

Symptoms	Probable Causes and Solutions
Shaker does not run.	Power cord is not plugged in and/or power switch is off: plug in power cord (to working electric outlet), and turn on power switch.
	On/Off switch is not working: call for service.
	Blown fuse: call for service.
	Defective main board: call for service.
	Defective display controller board: call for service.
	Jammed shaking mechanism: call for service.
	Defective motor: call for service.
	Drive belt out of alignment or worn: call for service.
Shaker runs slowly and/or no speed indication.	Blown fuse: call for service.
	Drive belt out of alignment or worn: call for service.
	Incorrect speed calibration: call for service
	Defective main board: call for service.
	Defective motor: call for service.
Shaker does not run at set speed.	Defective motor: call for service.
	Shaker is overloaded and/or you are using baffled flasks: remove some contents and balance load.
	Drive belt out of alignment or worn: call for service.
Operating noise	Load out of balance: unload all contents, then reload.
	Loose components in platform, subplatform and/or drive assembly: call for service.

Troubleshooting

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

8 Maintenance

8.1 Cleaning external surfaces



WARNING!

- ▶ Always turn off the shaker and disconnect the power cord from the power supply before performing any maintenance on the shaker.
 - ▶ A detachable main power cord has been provided with your unit. Only use the cord provided and do not replace cord with an inadequately rated cord.
-

Use a cloth dampened with water or any standard, household or laboratory cleaner to wipe down the shaker's outer surfaces.

Never use abrasive or corrosive compounds to clean this instrument, as they may damage the shaker and void the warranty.

Maintenance

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

9 Technical data

9.1 Specifications

Shaking	
Speed	50 rpm – 400 rpm
Motion	2.54 cm (1 in)
Indication	LED digital electric display, 1 rpm increments
Setpoint and Control	Digital adjustment with PI microprocessor control and instantaneous visual feed back ± 1 rpm.
Accuracy	± 2 rpm
Drive	
UniCentric™ single eccentric counterbalanced ball bearing drive	
Keypad timer	
<ul style="list-style-type: none"> • Programmable shaking periods from 0.1 – 99.9 h by a digital timer that shuts off at the end of period and energizes status light. • Timer counts down and digital display indicates remaining time. • Can be deactivated for continuous operation. • Additionally, shaker will display total accumulated running time for service information. 	
Operating ambient environment	
<ul style="list-style-type: none"> • 5 – 45 °C • 20 – 80 % humidity, non-condensing • Up to 2000 m 	
Alarms	
<ul style="list-style-type: none"> • Warning signal (audible and visible) indicates when shaking speed deviates more than ± 5 rpm from setpoint and when timer operation has expired. • Audible alarm can be deactivated/activated by the operator. 	
Automatic restart	
<ul style="list-style-type: none"> • Shaker will automatically restart after undesired power interruption. • Setpoints are maintained by non-volatile memory. • Interruption is indicated by a flashing display. 	
Electrical service	
<ul style="list-style-type: none"> • 110V/120V AC, 50/60 Hz, 1320 VA • 220V/240V AC, 50/60 Hz, 1320 VA 	

Technical data

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Dimensions	
Width	76 cm (30 in)
Depth	68.3 cm (27 in)
Height	17.3 cm (7 in)

Platform dimensions	
Width × Depth	76 cm (30 in) × 46 cm (18 in)

Weight	
Net	49 kg (108 lb)
Gross	66 kg (145 lb)

10 Ordering information

10.1 Parts and accessories

When ordering replacement or accessory parts, or requesting service, please provide the Model Number and Serial Number of your shaker. This information is on the **ELECTRICAL SPECIFICATION PLATE** located on the side panel of the shaker.

10.1.1 Belt replacement parts

Part description	Quantity	Part number
V-Belt	1	R-334
3/8-16 NC x 1 1/4 in flat head Allen screw	3	S1127

10.1.2 Dedicated platforms

Platform description	Flask capacity	Part number
50 ml Erlenmeyer Flasks	108	M1119-9908
125 ml Erlenmeyer Flasks	60	M1191-9909
250 ml Erlenmeyer Flasks	40	M1191-9910
500 ml Erlenmeyer Flasks	24	M1191-9911
1 L Erlenmeyer Flasks	15	AG-1
2 L Erlenmeyer Flasks	12	AG-2
2.8 L Fernbach Flasks	6	AG-28
4 L Erlenmeyer Flasks	6	AG-4
6 L Erlenmeyer Flasks	4	AG-6

10.1.3 Universal platform flask capacity

The Universal Platform (Part Number M1250-9920) is capable of holding the following quantities of flasks:

Flask type	Capacity
50 ml Erlenmeyer Flasks	91
125 ml Erlenmeyer Flasks	39
250 ml Erlenmeyer Flasks	30
500 ml Erlenmeyer Flasks	18
1 L Erlenmeyer Flasks	12
2 L Erlenmeyer Flasks	8
2.8 L Fernbach Flasks	6
4 L Erlenmeyer Flasks	6

Ordering information

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Flask type	Capacity
6 L Erlenmeyer Flasks	4

10.1.4 Racks and trays

Accessory description	New Brunswick part number	Platform capacity	
Adjustable angle test tube rack for tubes 8 – 11 mm diameter	80 tube capacity	M1289-0100	7
	60 tube capacity	M1289-0010	9
	48 tube capacity	M1289-0001	9
Adjustable angle test tube rack for tubes 12 – 15 mm diameter	60 tube capacity	M1289-0200	7
	44 tube capacity	M1289-0020	9
	34 tube capacity	M1289-0002	9
Adjustable angle test tube rack for tubes 15 – 18 mm diameter	42 tube capacity	M1289-0300	7
	31 tube capacity	M1289-0030	9
	24 tube capacity	M1289-0003	9
Adjustable angle test tube rack for tubes 18 – 21 mm diameter	30 tube capacity	M1289-0400	7
	23 tube capacity	M1289-0040	9
	18 tube capacity	M1289-0004	9
Adjustable angle test tube rack for tubes 22 – 26 mm diameter	22 tube capacity	M1289-0500	7
	16 tube capacity	M1289-0050	9
	13 tube capacity	M1289-0005	9
Adjustable angle test tube rack for tubes 26 – 30 mm diameter	20 tube capacity	M1289-0600	7
	16 tube capacity	M1289-0060	9
	12 tube capacity	M1289-0006	9
Microplate holder rack (stacked)	3 deep well or 9 standard	M1289-0700	16
Microplate holder rack 5 deep well or standard TTR-221 4 (single layer)	5 deep well or standard	TTR-221	4
Angled test tube rack holder* for user-supplied test tube racks that are 10 – 13 mm (4 – 5 in) wide and up to 38 mm (15 in) long.	TTR-210	4	
Angled test tube rack spacer bar* for use with TTR-210 to accommodate test tubes racks that are less than 13 mm (5 in) wide.	TTR-215	N/A	

*Universal Platform Required

11 Transport, storage and disposal

11.1 Disposal

In case the product is to be disposed of, the relevant legal regulations are to be observed.

Information on the disposal of electrical and electronic devices in the European Community:

Within the European Community, the disposal of electrical devices is regulated by national regulations based on EU Directive 2012/19/EU pertaining to waste electrical and electronic equipment (WEEE).

According to these regulations, any devices supplied after August 13, 2005, in the business-to-business sphere, to which this product is assigned, may no longer be disposed of in municipal or domestic waste. To document this, they have been marked with the following identification:



Because disposal regulations may differ from one country to another within the EU, please contact your supplier if necessary.

In Germany, this is mandatory from March 23, 2006. From this date, the manufacturer has to offer a suitable method of return for all devices supplied after August 13, 2005. For all devices supplied before August 13, 2005, the last user is responsible for the correct disposal.

Transport, storage and disposal

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

12 Declaration of conformity

The E-10 Shaker has been tested to the appropriate standards as attested in the following Declaration of Conformity.

eppendorf

Declaration of Conformity

The product named below fulfills the requirements of directives and standards listed. In the case of unauthorized modifications to the product or an unintended use this declaration becomes invalid.

Product name:

Excella® E10
including accessories

Product type:

Benchtop open air shaker

Relevant directives / standards:

2006/95/EC: EN 61010-1, CAN/CSA-C22.2 No. 61010-1-12, UL-61010-1
2004/108/EC: EN 61326-1, EN 61000-3-2, EN 61000-3-3
2011/65/EU
2012/19/EU



Management Board



Portfolio Management

Date: November 22, 2013

Your local distributor: www.eppendorf.com/contact
Eppendorf AG · 22331 Hamburg · Germany
eppendorf@eppendorf.com

ISO 9001
Certified

ISO 13485
Certified

ISO 14001
Certified

M1351-2115-00

Eppendorf and the Eppendorf Logo are registered trademarks of Eppendorf AG Hamburg/Germany.
All rights reserved incl. graphics and pictures. Copyright 2013 © by Eppendorf AG.

www.eppendorf.com

Declaration of conformity

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Index

A

Alarm functions22

Audible alarm22

Auto restart function22

C

Clamp

Double girdle clamp14

Clamp installation13

Cleaning27

Connecting to mains/power15

Control panel17

D

Danger level5

CAUTION5

DANGER5

NOTICE5

WARNING5

Declaration of conformity35

Disposal33

F

Flask clamp installation13

Function indicators18

I

Installing platform12

M

Maintenance27

Manual conventions5

Mute alarm22

P

Parts

Dedicated platforms31

Platform12

Platforms

Dedicated platforms31

Power failure22

S

Speed calibration23

Status indicators17

Symbols used5

T

Trouble shooting guide25

U

Using this manual5

Index

New Brunswick Excella® E-10 Open Air Shaker
English (EN)

Evaluate your manual

Give us your feedback.
www.eppendorf.com/manualfeedback